

# Validation of segmental bio-electrical impedance analysis to assess sarcopenia in older adults

**Author(s)**

van den Helder, J.E.M.; Jansen, I.; Kruijning, S.; van Dronkelaar, D.C.; Engelbert, R.H.H.; Weijs, P.J.M.; Tieland, C.A.B.

**Publication date**

2017

**Document Version**

Final published version

**License**

CC BY

[Link to publication](#)

**Citation for published version (APA):**

van den Helder, J. E. M., Jansen, I., Kruijning, S., van Dronkelaar, D. C., Engelbert, R. H. H., Weijs, P. J. M., & Tieland, C. A. B. (2017).

*Validation of segmental bio-electrical impedance analysis to assess sarcopenia in older adults*. Poster session presented at 39th ESPEN congress, The Hague, Netherlands.

**General rights**

It is not permitted to download or to forward/distribute the text or part of it without the consent of the author(s) and/or copyright holder(s), other than for strictly personal, individual use, unless the work is under an open content license (like Creative Commons).

**Disclaimer/Complaints regulations**

If you believe that digital publication of certain material infringes any of your rights or (privacy) interests, please let the Library know, stating your reasons. In case of a legitimate complaint, the Library will make the material inaccessible and/or remove it from the website. Please contact the library: <https://www.amsterdamuas.com/library/contact/questions>, or send a letter to: University Library (Library of the University of Amsterdam and Amsterdam University of Applied Sciences), Secretariat, Singel 425, 1012 WP Amsterdam, The Netherlands. You will be contacted as soon as possible.

# Validation of segmental bio-electrical impedance analysis to assess sarcopenia in older adults

J. van den Helder<sup>1,2</sup>, I. Jansen<sup>1</sup>, S. Kruijning<sup>1</sup>, C. van Dronkelaar<sup>1</sup>, R.H.H. Engelbert<sup>2,3</sup>, P.J.M. Weijs<sup>1,4</sup>, M. Tieland<sup>1</sup>

<sup>1</sup> Faculty of Sports and Nutrition, Amsterdam University of Applied Sciences, Amsterdam, The Netherlands; <sup>2</sup> Amsterdam Center for Innovative Health Practice (ACHIEVE), Faculty of Health, Amsterdam University of Applied Sciences, Amsterdam, The Netherlands; <sup>3</sup> Department of Rehabilitation, Academic Medical Center, Amsterdam, The Netherlands; <sup>4</sup> Department of Nutrition and Dietetics, Internal Medicine, VU University Medical Center, Amsterdam, The Netherlands

## Rationale

Sarcopenia is an age-related decrease of muscle mass and strength and is assessed by dual energy X-ray absorptiometry (DXA) using appendicular fat free mass (aFFM). Besides DXA, an easy, cheap and feasible technique to measure aFFM is bio-electrical impedance analysis (BIA). The aim of this study was to validate aFFM measurements of BIA with DXA.

## Methods

Appendicular FFM in older adults was assessed by BIA (Tanita MC-780 MA; 8-polar) and DXA (Hologic A). Participants were included in the VITAMIN trial. Pearson-correlation was used to determine correlation between the aFFM of the BIA and DXA. Paired t-test was used to compare the two techniques. Agreement between the two techniques was assessed by the Bland-Altman plot.

**Table 1. Characteristics of population**

Characteristics of population	Total (n=45)
Age, mean (SD), years	72 (6.7)
Sex, n (%)	
- Women	39 (86.7)
- Men	6 (13.3)
Ethnicity, n (%)	
- Caucasian/white	44 (97.8)
- Black	1 (2.2)
Weight, mean (SD), kg	71.8 (9.5)
Height, mean (SD), cm	165.1 (7.8)

## Results

Table 1 shows the characteristics of 45 older adults with a mean age of 72 ± 6.7 years. Table 2 shows data analysis of aFFM assessment for BIA and DXA. Significant association was found for aFFM of BIA with aFFM of DXA ( $r = 0.934$ ,  $p < 0.0001$ ). Appendicular FFM by BIA was significant lower by 2.2% compared to DXA ( $19.94 \pm 2.81$  vs  $20.38 \pm 3.33$ ,  $p = 0.019$ ).


**Table 2. Data analysis of appendicular FFM assessment of DXA - BIA**

	DXA	BIA	Δ BIA-DXA	Dependent t-test (p)	Pearson (ρ)
aFFM <sup>1</sup>	20.38 ± 3.33	19.94 ± 2.81	- 0.44 ± 1.22	0.019	0.934*
aFFM right arm <sup>1</sup>	2.50 ± 0.48	2.43 ± 0.39	- 0.07 ± 0.22	0.035	0.897*
aFFM left arm <sup>1</sup>	2.35 ± 0.49	2.49 ± 0.41	+ 0.14 ± 0.25	0.001	0.866*
aFFM right leg <sup>1</sup>	7.80 ± 1.23	7.53 ± 1.07	- 0.26 ± 0.50	0.001	0.914*
aFFM left leg <sup>1</sup>	7.73 ± 1.27	7.48 ± 1.01	- 0.25 ± 0.55	0.004	0.910*

<sup>1</sup> aFFM values in mean kg ± SD

\*  $p < 0.0001$

BIA underestimated aFFM with a mean difference of  $0.44 \pm 1.22$  kg according to the Bland-Altman plot (Figure 1). The positive regression line showed a significant proportional bias ( $\beta = 0.430$ ,  $p = 0.003$ ), suggesting that BIA underestimated aFFM in older adults with a high FFM. Bland-Altman plot showed wide limits of agreement (LoA -1.96, 2.84).

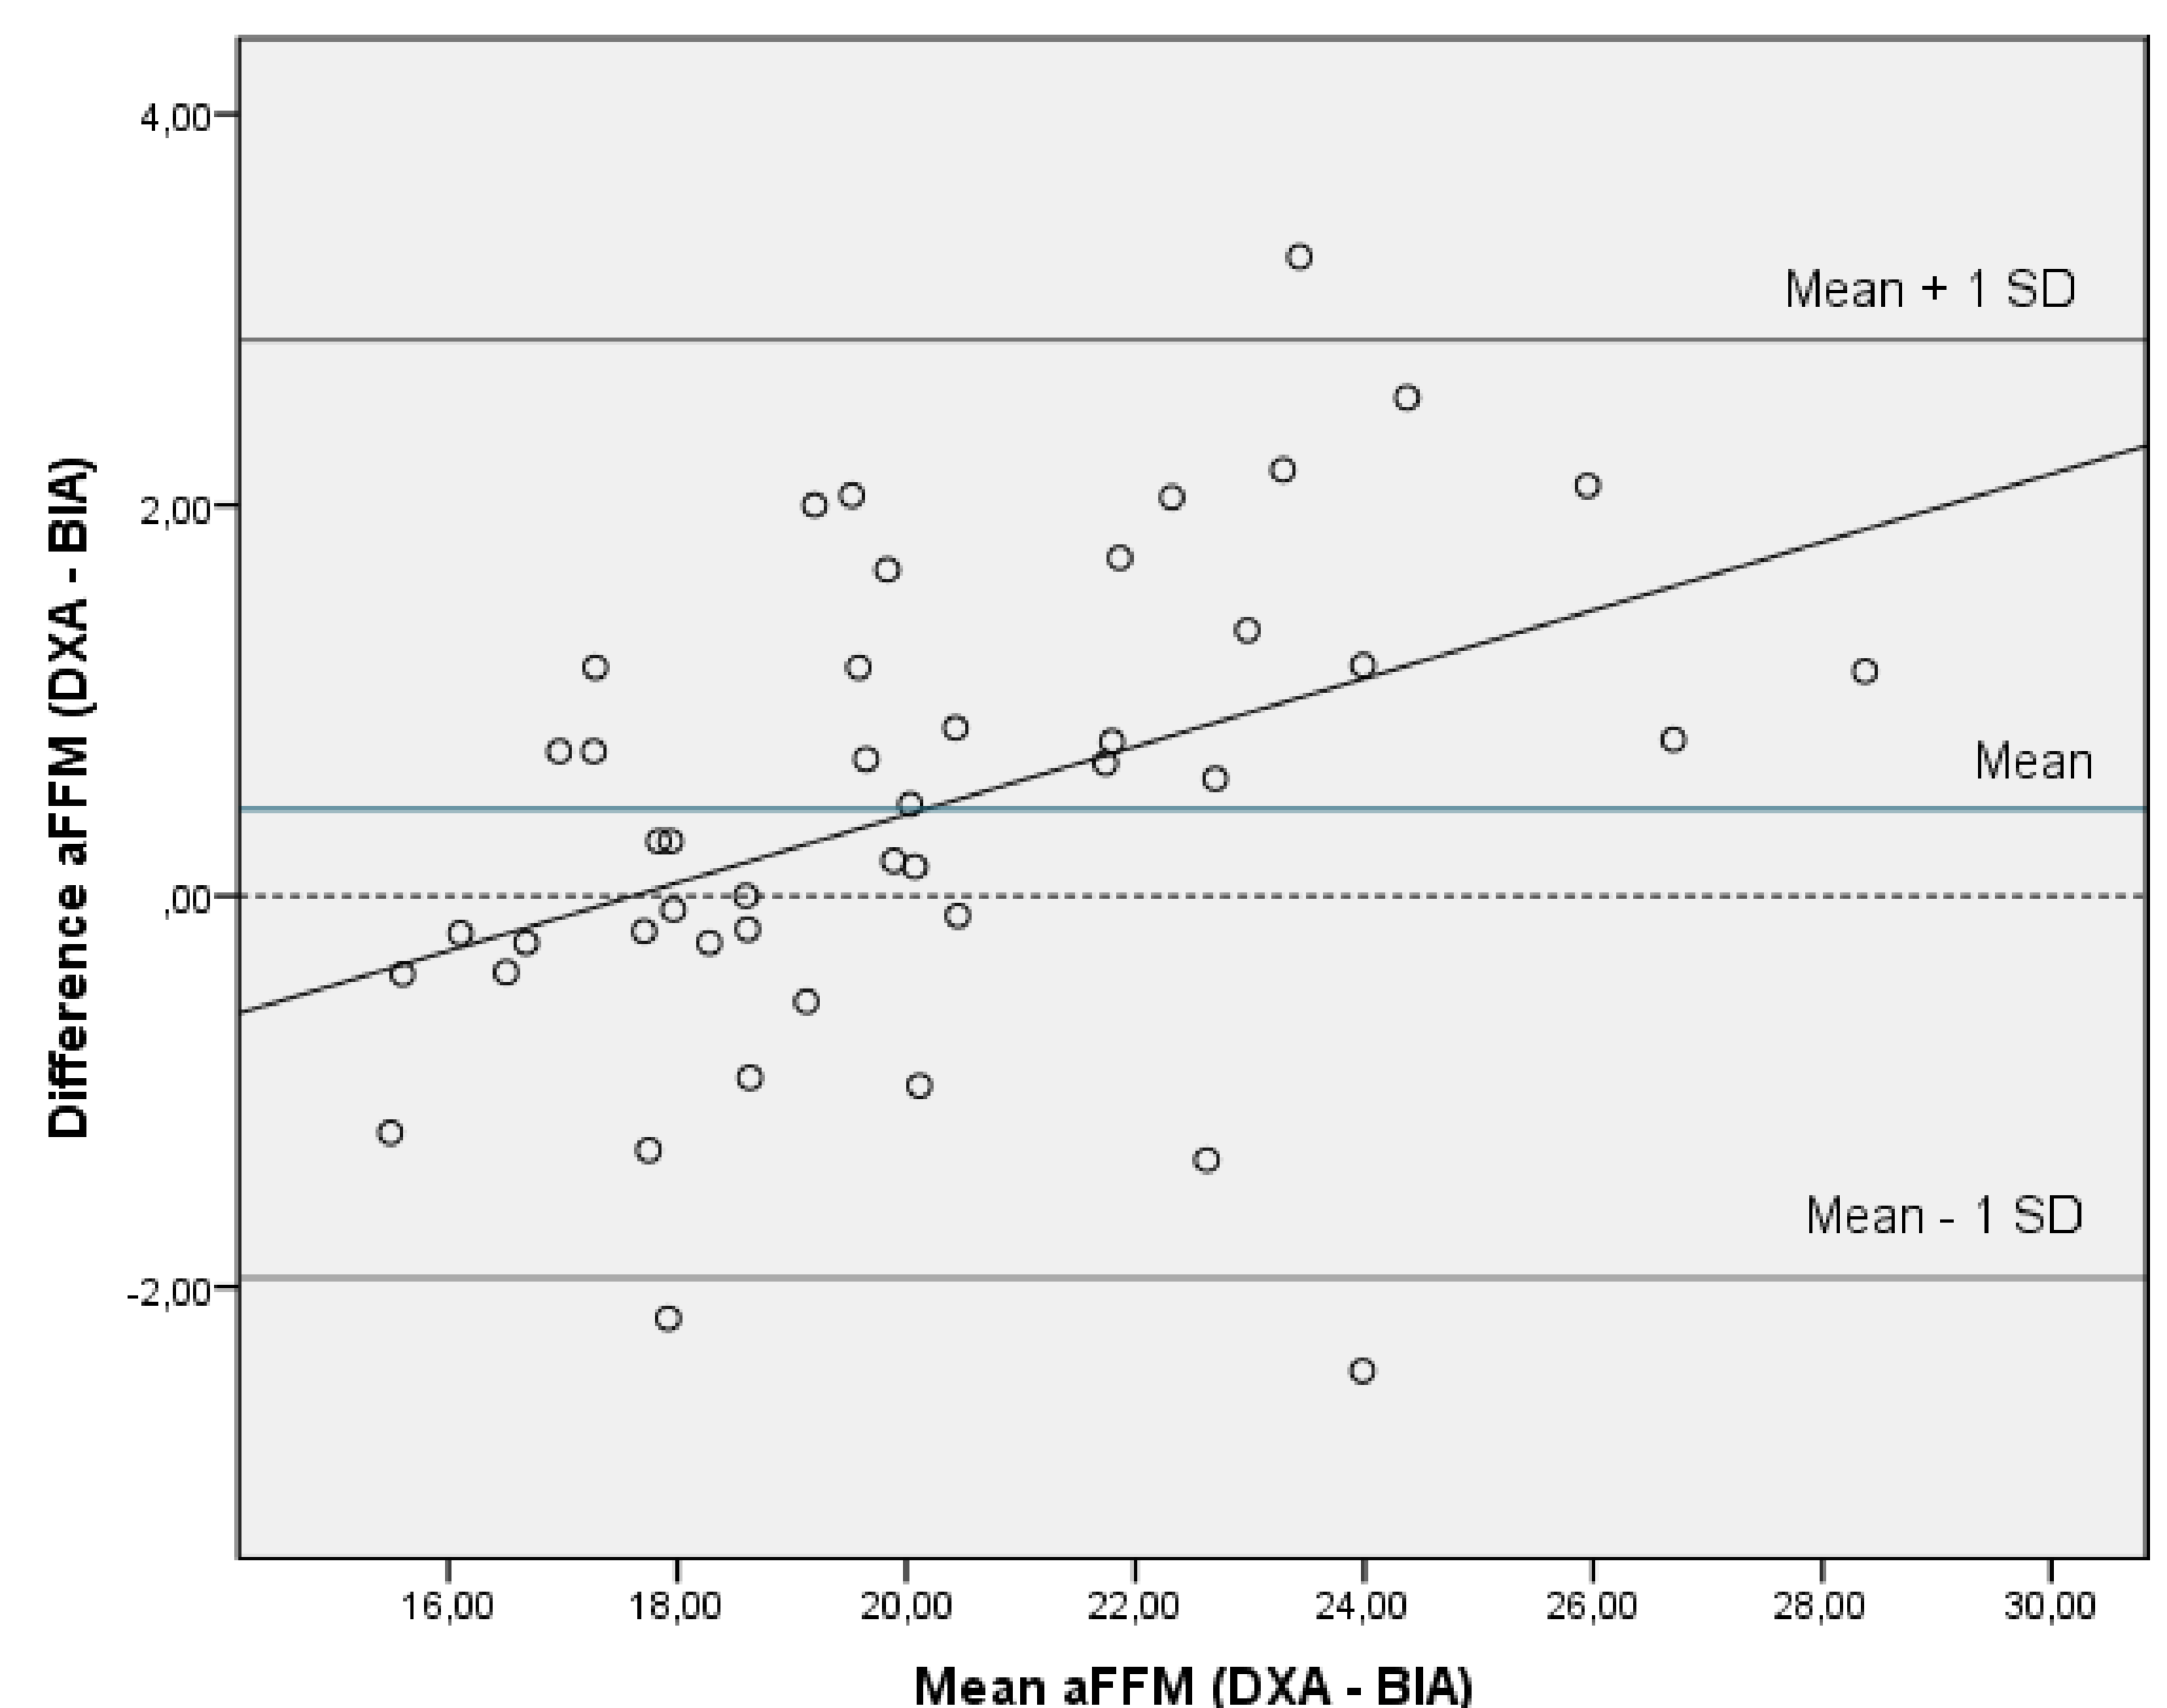

**Figure 1. Bland - Altman plot Appendicular FFM DXA - BIA**

## Conclusion

On a group level, the BIA may be accurate to assess aFFM in older adults. On an individual level, however, the variation between BIA - DXA to assess aFFM is high. More research is necessary with a larger sample size.

## Correspondence

[j.e.m.van.den.helder@hva.nl](mailto:j.e.m.van.den.helder@hva.nl)/  
[vitamine@hva.nl](mailto:vitamine@hva.nl), Jantine van den Helder,  
Faculty of Sports and Nutrition, Amsterdam  
University of Applied Sciences, Dokter  
Meurerlaan 8, 1067 SM, Amsterdam, The  
Netherlands