

Amsterdam University of Applied Sciences

The effect of hydration status on intracellular and extracellular water using bioelectrical impedance analysis measurements

van Dronkelaar, C.; Verstappen, J.J.J. ; Memelink, R.G. ; Tieland, M.; Kruizenga, H.M. ; Weijs, P.J.M.

Publication date

2019

Document Version

Final published version

[Link to publication](#)

Citation for published version (APA):

van Dronkelaar, C., Verstappen, J. J. J., Memelink, R. G., Tieland, M., Kruizenga, H. M., & Weijs, P. J. M. (2019). *The effect of hydration status on intracellular and extracellular water using bioelectrical impedance analysis measurements*. Poster session presented at 15th International Congress of the European Geriatric Medicine Society, Kraków, Poland.

General rights

It is not permitted to download or to forward/distribute the text or part of it without the consent of the author(s) and/or copyright holder(s), other than for strictly personal, individual use, unless the work is under an open content license (like Creative Commons).

Disclaimer/Complaints regulations

If you believe that digital publication of certain material infringes any of your rights or (privacy) interests, please let the Library know, stating your reasons. In case of a legitimate complaint, the Library will make the material inaccessible and/or remove it from the website. Please contact the library:

<https://www.amsterdamuas.com/library/contact/questions>, or send a letter to: University Library (Library of the University of Amsterdam and Amsterdam University of Applied Sciences), Secretariat, Singel 425, 1012 WP Amsterdam, The Netherlands. You will be contacted as soon as possible.

The effect of hydration status on intracellular and extracellular water using bioelectrical impedance analysis measurements

C. van Dronkelaar^{1,2}, J.J.J. Verstappen^{1,2}, R.G. Memelink¹, M. Tieland¹, H.M. Kruizenga², P.J.M. Weijs^{1,2}

¹ Faculty of Sports and Nutrition, Center of Expertise Urban Vitality, Amsterdam University of Applied Sciences, Amsterdam, The Netherlands;
² Department of Nutrition and Dietetics, Amsterdam University Medical Centers, VU University, Amsterdam, The Netherlands.


Aim

The aim of the study was to assess whether measurements of intracellular water (ICW) and extracellular water (ECW) in the upper-leg are less sensitive to changes in hydration status than measurements of the whole body, using single- (SF) and multi-frequency (MF) bioelectrical impedance analysis (BIA). SF is only able to measure ECW at 50 kHz, whereas MF is able to measure both ECW and ICW using 5, 50 and 200 kHz.

Methods

The impedance of upper-leg and whole-body was measured in:

- 30 healthy adults, mean age 25.5±8.3yrs, 51.7% women
- ECW: Z_{50} (50 kHz; **SF-BIA**)
- ICW: $Z_{200-5} = 1/[(1/Z_{200}) - (1/Z_5)]$ (5kHz and 200kHz; **MF-BIA**)
- hydration states:
 - A** fasted with no use of the toilet
 - B** after use of toilet (reference state)
 - C** after toilet use and drinking 1 liter water

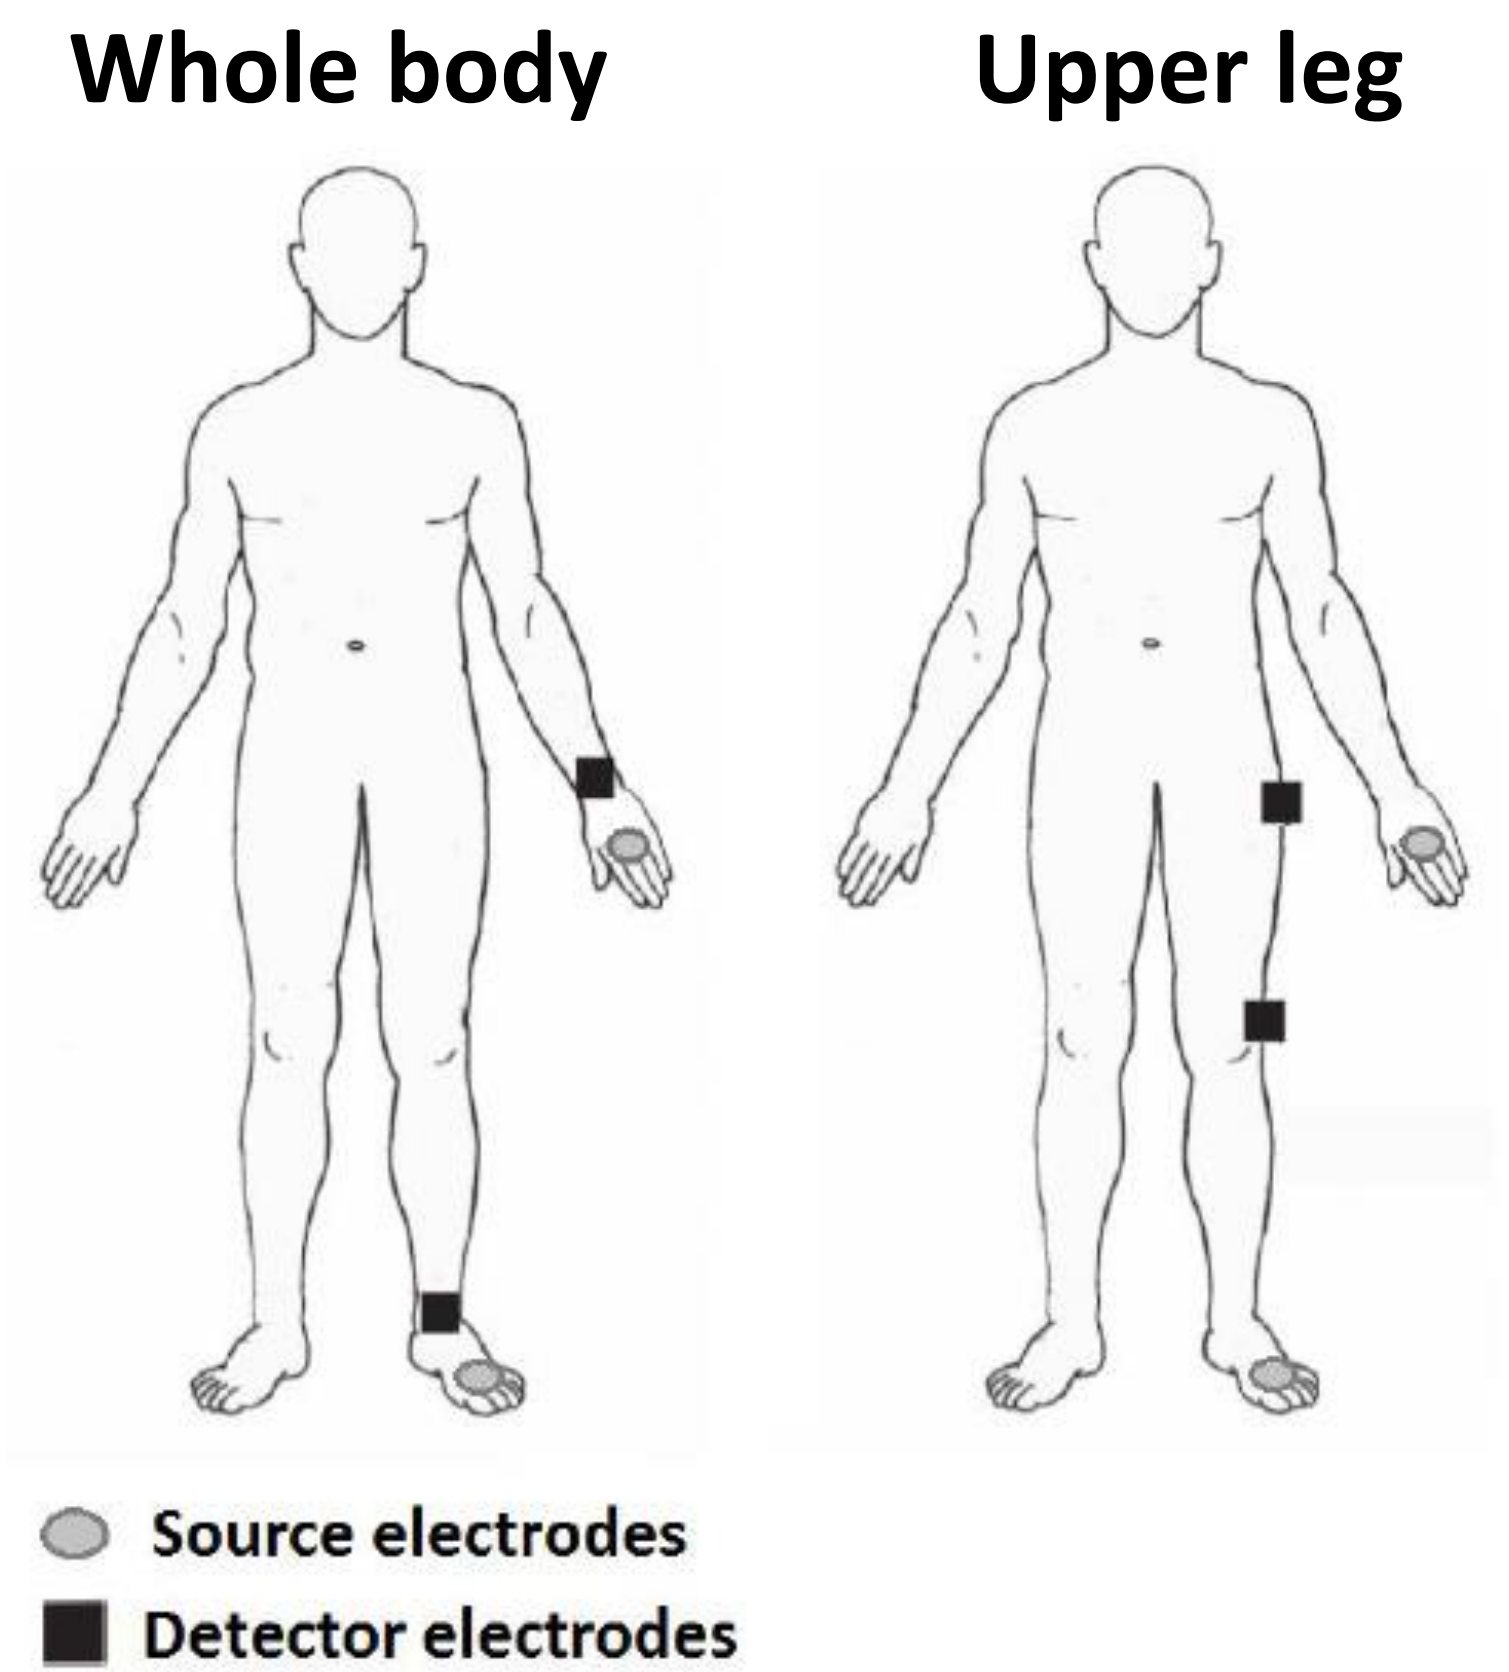

Main Findings

- Intracellular water was not influenced by hydration status, therefore *multi-frequency* BIA is preferred over *single-frequency* BIA to assess muscle mass.
- Upper-leg impedance was **not less sensitive** to changes in hydration status than whole –body impedance.

Results

ECW was significantly influenced by hydration status in both upper-leg and whole-body ($p < 0.01$). ICW was not significantly influenced by hydration status ($p > 0.05$), except for the upper leg measurement in situation A (without toilet use) ($p = 0.015$).

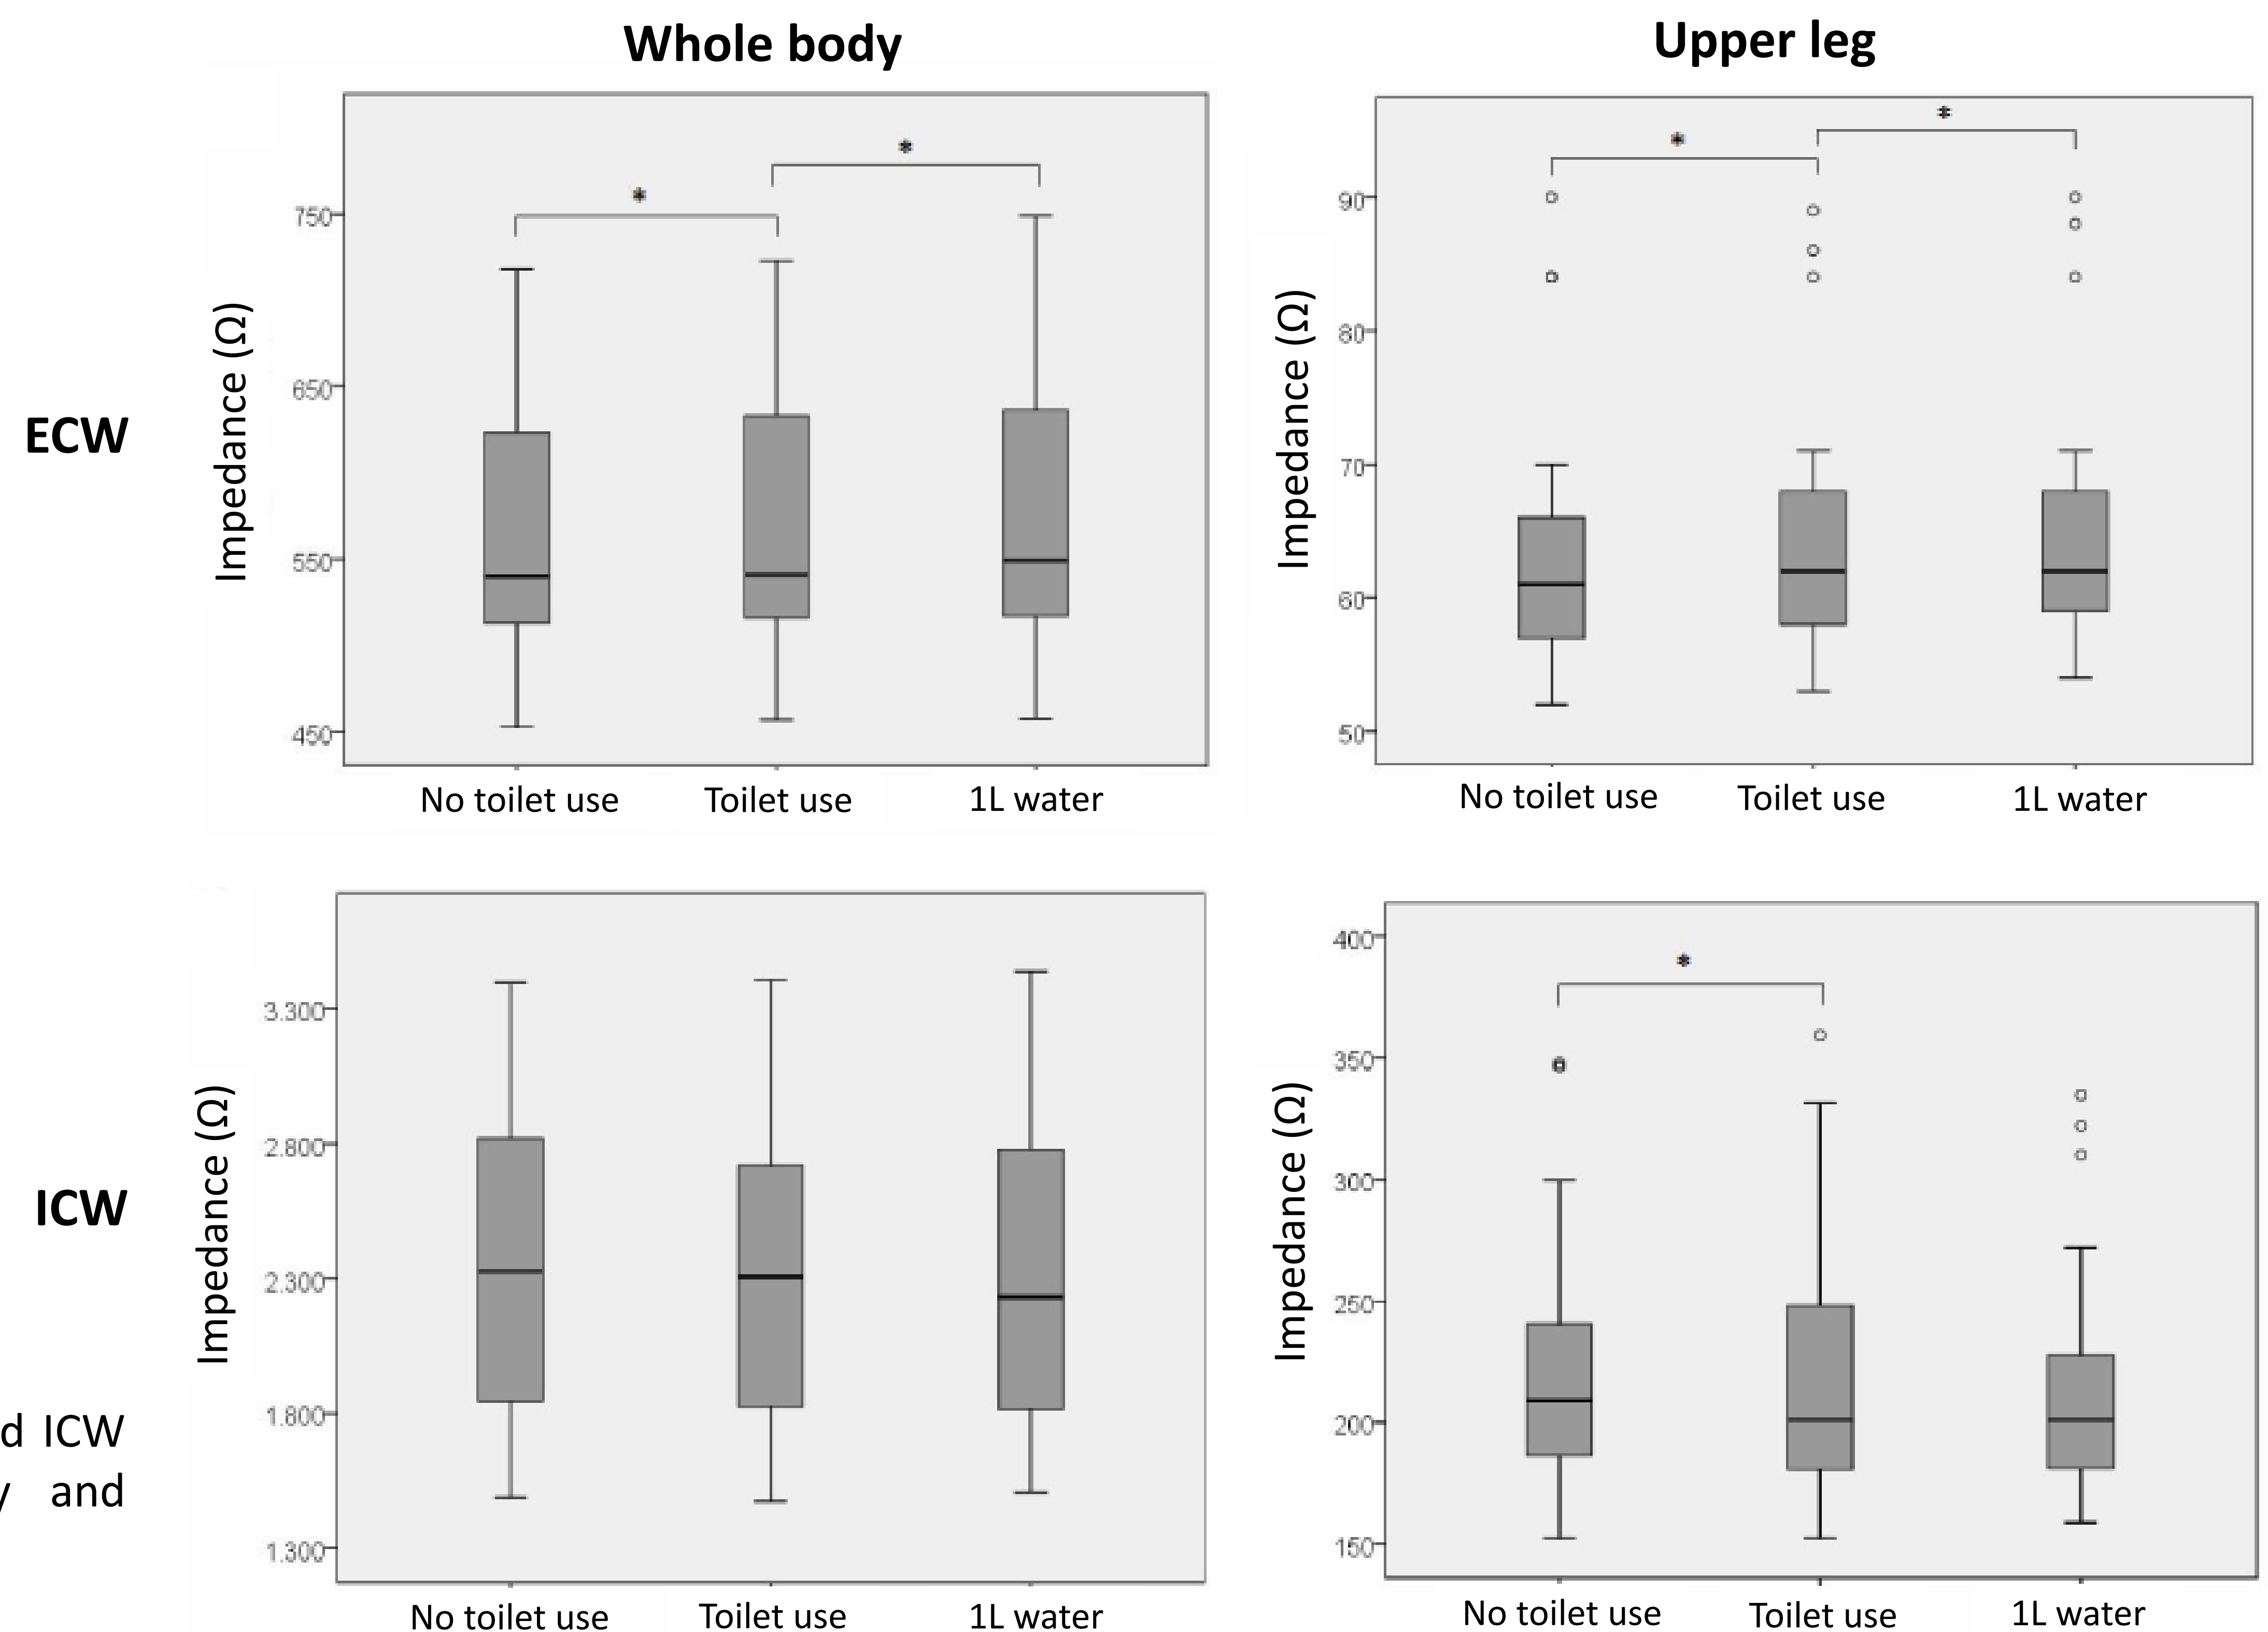


Figure 1. Boxplot of ECW and ICW impedance in whole body and upper leg. * $p < 0.05$

This study is part of the ProIntens multicenter study

Correspondence

Carliene van Dronkelaar / d.c.van.dronkelaar@hva.nl
Amsterdam University of Applied Sciences,
Dokter Meurerlaan 8,
1067SM Amsterdam, The Netherlands