

The diagnostic accuracy of headache measurement instruments

a systematic review and meta-analysis focusing on headaches associated with musculoskeletal symptoms

Author(s)

van der Meer, H.A.; Visscher, C.M.; Vredeveld, T.; Nijhuis-van der Sanden, M.W.G.; Engelbert, R.H.H.; Speksnijder, C.M.


Publication date

2019

[Link to publication](#)

Citation for published version (APA):

van der Meer, H. A., Visscher, C. M., Vredeveld, T., Nijhuis-van der Sanden, M. W. G., Engelbert, R. H. H., & Speksnijder, C. M. (2019). *The diagnostic accuracy of headache measurement instruments: a systematic review and meta-analysis focusing on headaches associated with musculoskeletal symptoms*. Poster session presented at American Academy for Orofacial Pain (AAOP) Scientific Meeting , San Diego, California, United States.

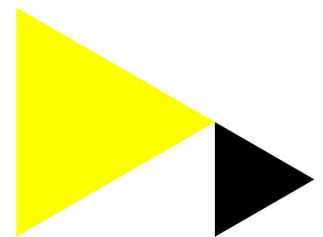

General rights

It is not permitted to download or to forward/distribute the text or part of it without the consent of the author(s) and/or copyright holder(s), other than for strictly personal, individual use, unless the work is under an open content license (like Creative Commons).

Disclaimer/Complaints regulations

If you believe that digital publication of certain material infringes any of your rights or (privacy) interests, please let the Library know, stating your reasons. In case of a legitimate complaint, the Library will make the material inaccessible and/or remove it from the website. Please contact the library: <https://www.amsterdamuas.com/library/contact/questions>, or send a letter to: University Library (Library of the University of Amsterdam and Amsterdam University of Applied Sciences), Secretariat, Singel 425, 1012 WP Amsterdam, The Netherlands. You will be contacted as soon as possible.

The Diagnostic Accuracy of Headache Measurement Instruments: A Systematic Review and Meta-Analysis focusing on Headaches associated with Musculoskeletal Symptoms

H.A. van der Meer¹⁻⁵, C.M. Visscher², T. Vredeveld¹, M.W.G. Nijhuis-van der Sanden⁵, R.H.H. Engelbert^{1,4}, C.M. Speksnijder³


AIM

To systematically review the available literature on the diagnostic accuracy of questionnaires and measurement instruments for headaches associated with musculoskeletal factors.

Headaches in this review:


- ❖ migraine;
- ❖ tension-type headache (TTH);
- ❖ cervicogenic headache (CGH);
- ❖ headache attributed to TMD (HATMD);
- ❖ headache attributed to whiplash.

- Associated with musculoskeletal factors:
- ✓ Decreased muscle function
 - ✓ Limited range of motion
 - ✓ Trigger points

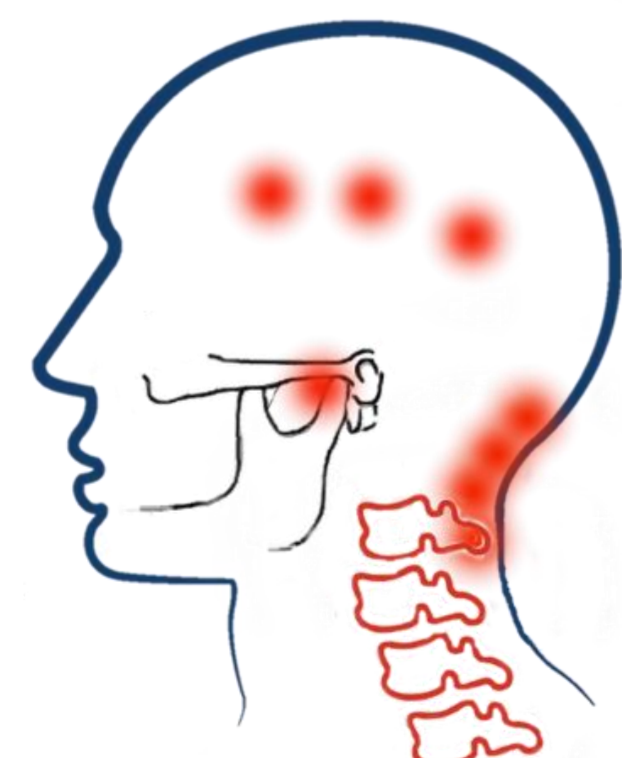

Registration: PROSPERO (CRD42017062472)

METHODS

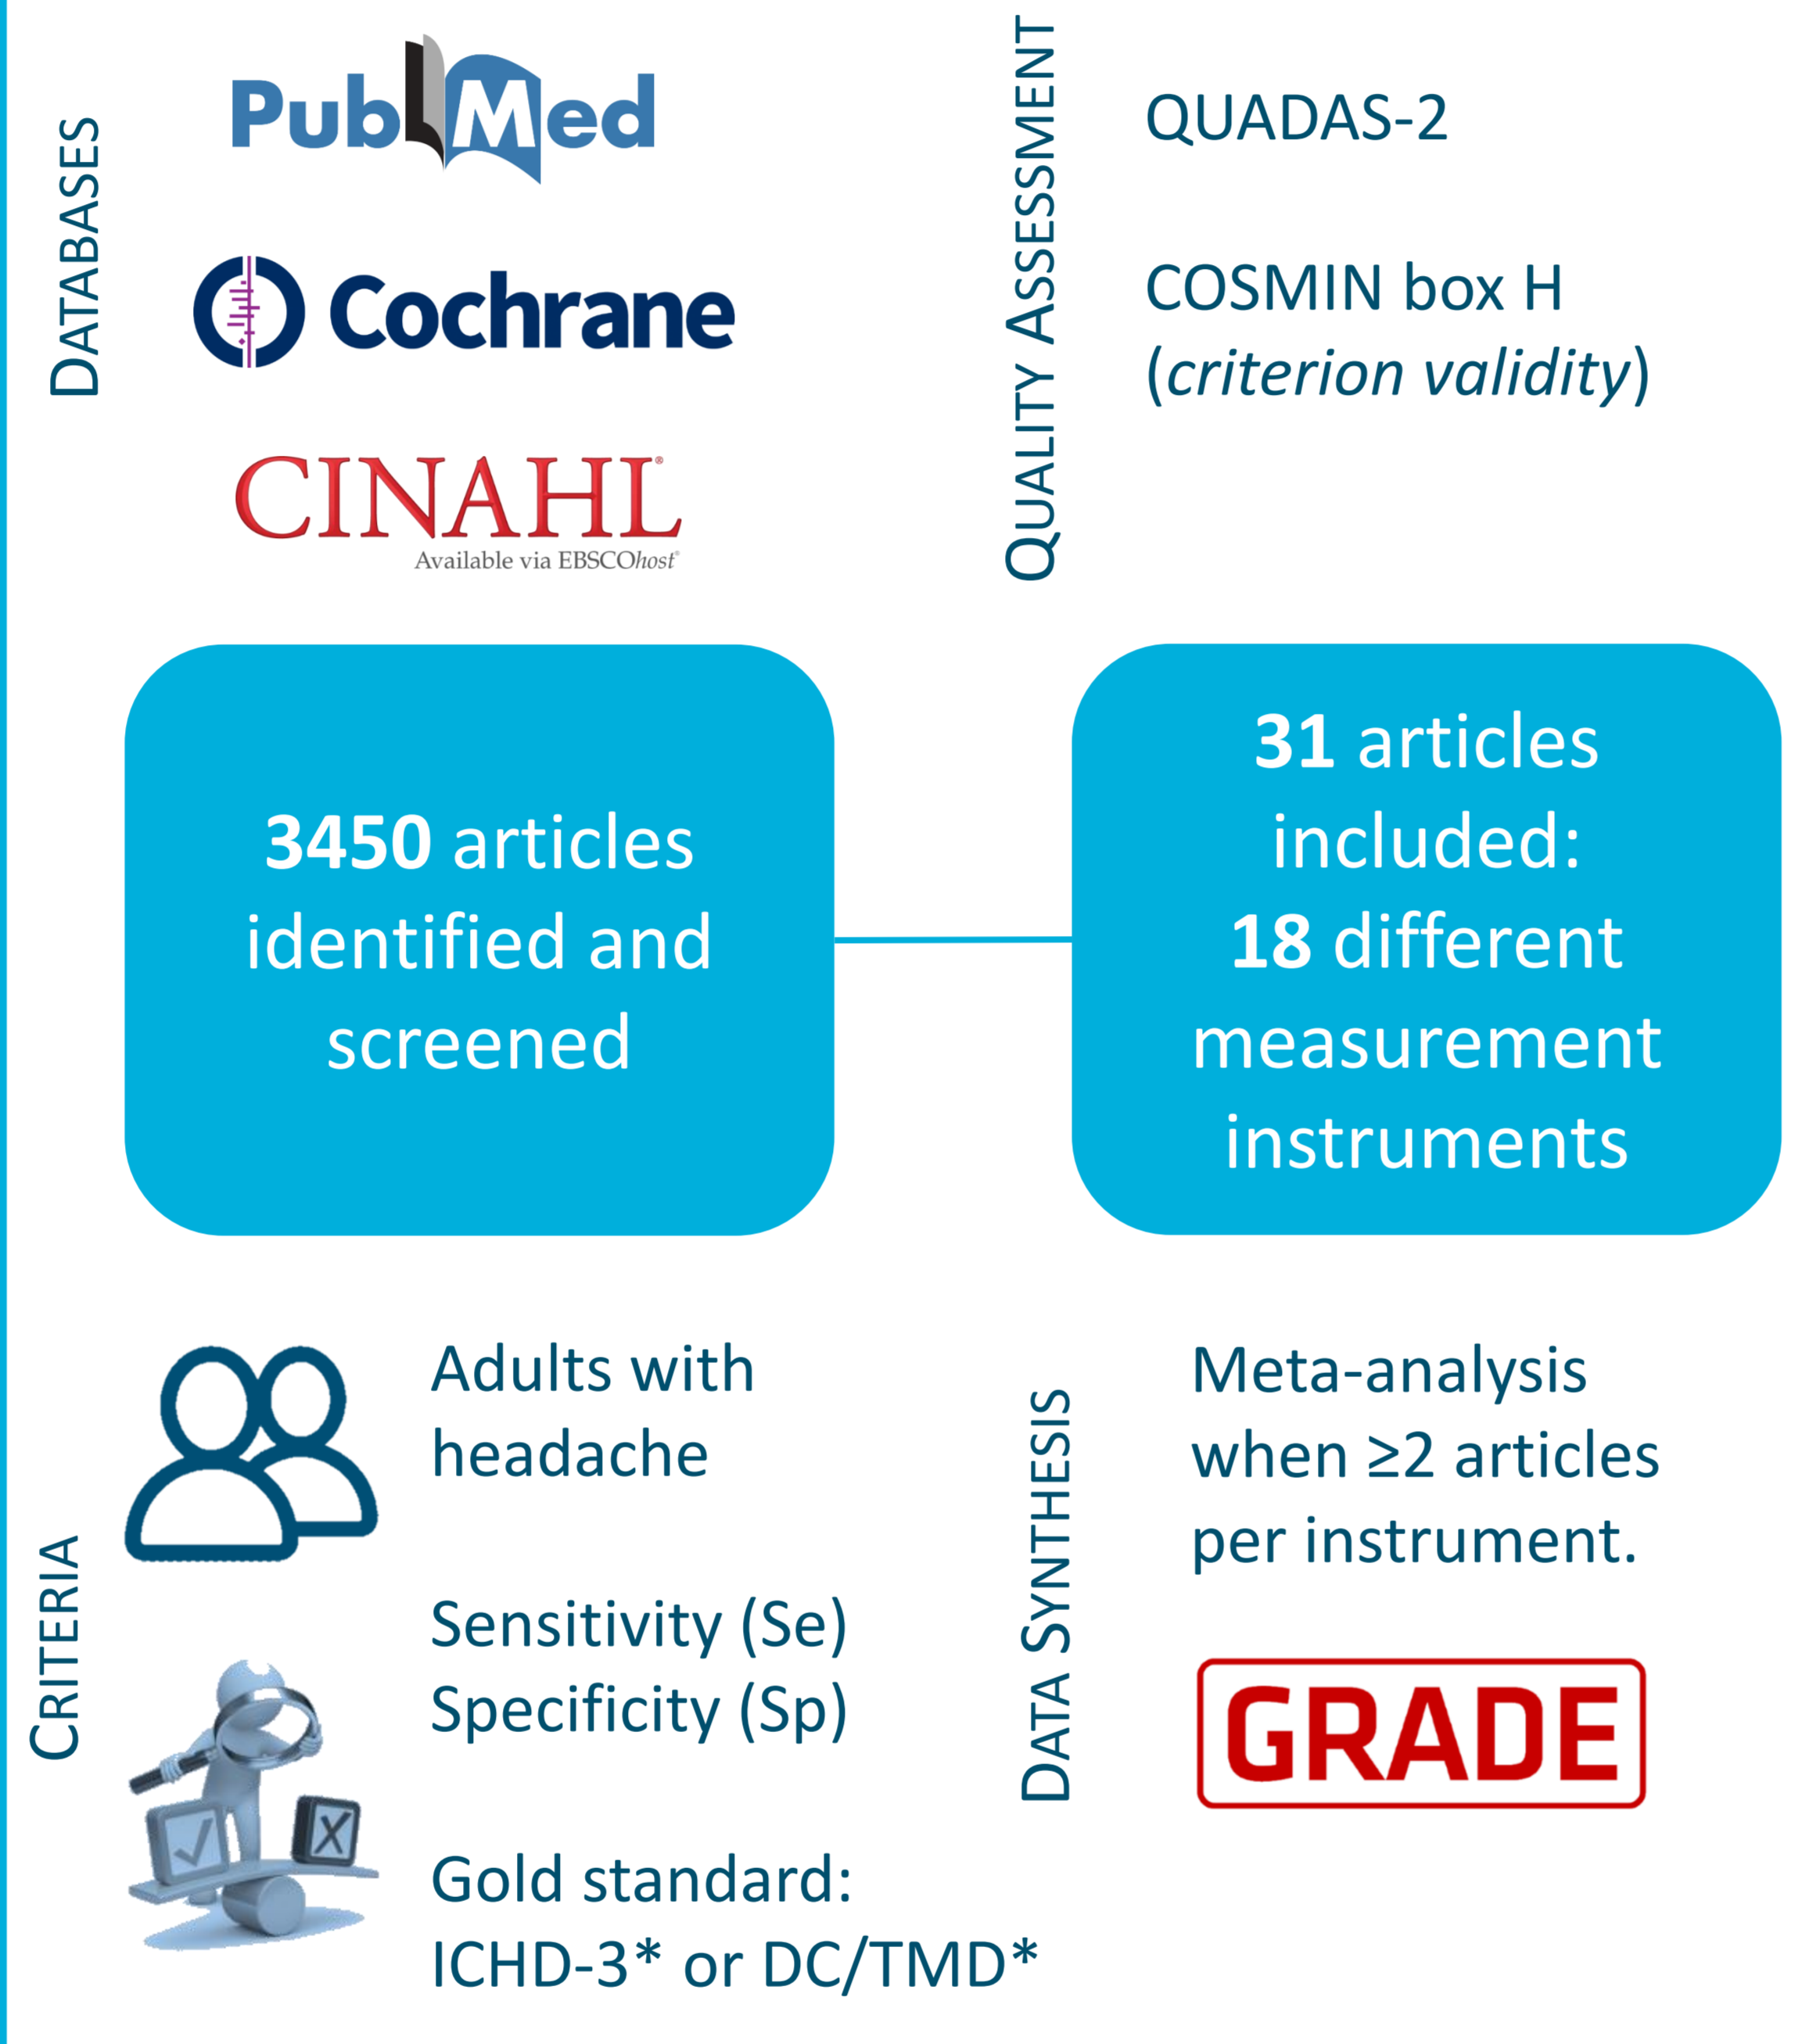

RESULTS

- No instruments for HATMD or headache attributed to whiplash.
- Se: Sensitivity; Sp: Specificity; M: Migraine; T: TTH

Migraine + TTH


German Headache Q
2 studies

Se 69%(M), 81%(T);
Sp 90%(M), 96%(T)
⊕⊕○○

Headache Screening Q (HSQ; 1 study)

Se 69%(M), 36%(T);
Sp 90 (M), 86%(T)
⊕⊕⊕○

Number of measurement instruments in this review per headache type:

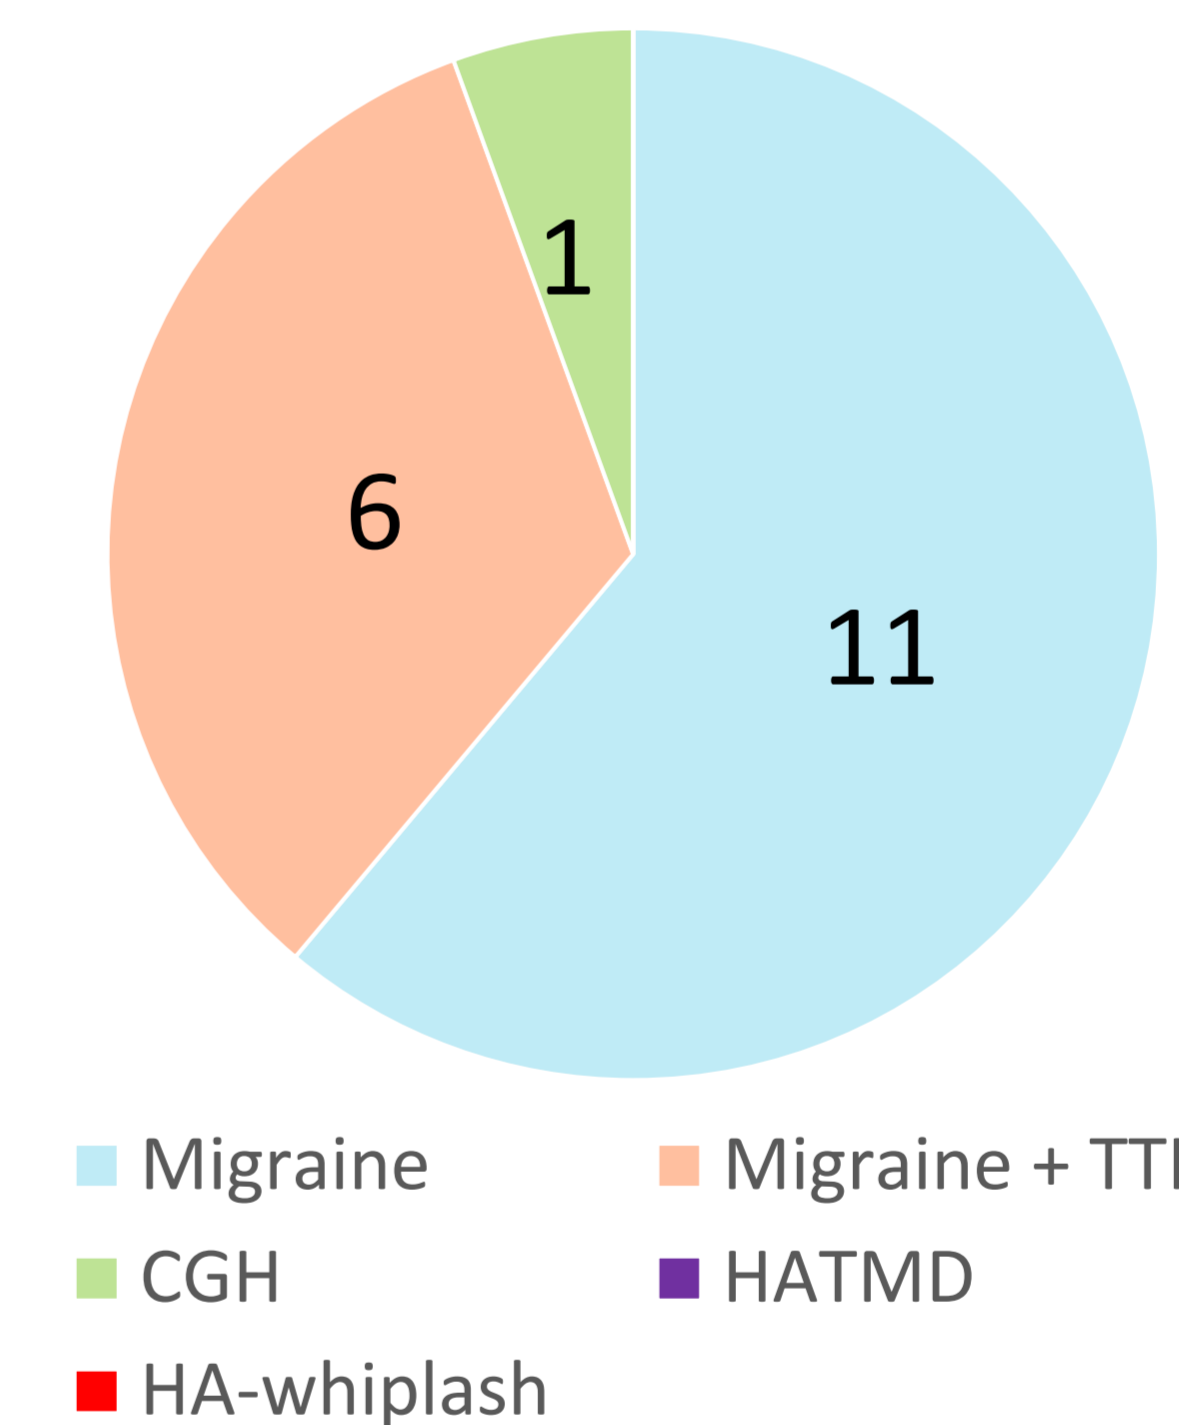

CGH

Cervical Flexion Rotation Test (CFRT) 2 studies

Se 83%; Sp 82%
⊕○○○

Migraine

ID-Migraine
9 studies

Se 87%; Sp 75%
⊕⊕⊕○

3 Question Screen
2 studies

Se 73%; Sp 93%
⊕⊕○○

TAKE HOME MESSAGE

- ✓ For migraine, the ID-Migraine is recommended (moderate level of certainty)
- ✓ For **migraine & TTH**, the HSQ is recommended (moderate level of certainty)
- ✓ For **CGH**, the CFRT is recommended (very low level of certainty)
- ✓ No measurement instruments available for headache attributed to TMD and whiplash trauma

References included studies:



***ICHD-3**: International Classification for Headache Disorders
***DC/TMD**: Diagnostic Criteria for Temporomandibular Disorders

Funding:
NWO
Netherlands Organisation for Scientific Research

This paper has been accepted for publication in *Cephalalgia*

¹ **Hogeschool van Amsterdam**
Amsterdam University of Applied Sciences

² **ACTA**

³ **UMC Utrecht**

Contact: h.a.van.der.meer@hva.nl

⁴ **Amsterdam UMC**
Universitair Medische Centra

Twitter: @HedwigFysio

⁵ **Institute for Health Sciences Radboudumc**